



Article	OR Gown, Mediwell light with Reinforcement, Standard Performance
Specification No.	46 44 37C
Article No.	46 44 37 , sterile goods 46 44 37-9 non-sterile goods
1. Description	OR Gown made of Mediwell light and with Mediwell light reinforcement, on the inside of the front and sleeves. The OR Gown and two hand towels are supplied in an overwrap in sterilisation packaging .
2. Application	For procedures without a particularly high fluid incidence.
3. Production	The above mentioned product is manufactured in hygienic conditions.
4. Material composition	<i>all of the materials used are latex-free!</i>
4.1 <u>Mediwell light</u>	
• Nonwoven	polypropylene nonwoven, turquoise
4.2 Cuff	synthetic fibre
4.3 <u>Sleeves & Front reinforcement / Mediwell light</u>	
• Nonwoven	polypropylene nonwoven, turquoise
• Lamination	glued lamination
4.4 <u>Included loose</u>	
• Hand towel 2x	# 62 40 40 PET-fadenverstärker Zellstoff
5. Product properties	fluid and alcohol repellent, high air permeability, highly comfortable to wear, low-lint.
6. Technical data	
6.1 <u>Dimensions</u>	
• Size	X-large
• Length	150 cm ± 5 cm
6.1.1 <u>Cuff</u>	
• Length	8 cm ± 2 cm

Quality Assurance:

Date: 07.07.2022

Signature: *Pöcher*



Article OR Gown, Mediwell light
with Reinforcement, Standard Performance

Specification No. **46 44 37C**

6.1.2 *Reinforcement / inside chest*

- Length 75 cm \pm 2 cm
- Width 50 cm \pm 2 cm

6.1.3 *Reinforcement / inside sleeves*

- Length 40 cm \pm 2 cm, *from the cuff*

6.1.4 *Final folded dimensions* 17 x 20 cm \pm 3 cm

6.1.5 *Included loose*

- Hand towel **2x**
- Length 39.5 cm \pm 2 cm
- Width 30 cm \pm 1 cm

6.2 *Raw material*

- *Nonwoven*
- Basis weight 35 g/m² \pm 10 %

6.3 *Performance requirements*

- The material used to make this product exceeds the minimum requirements, in accordance with the pertinent parts of EN 13795.
- Individual values can be found in the corresponding material specification.


The raw materials used in manufacture are physiologically harmless.



Article OR Gown, Mediwell light
with Reinforcement, Standard Performance

Specification No. 46 44 37C

7. Schematic diagram

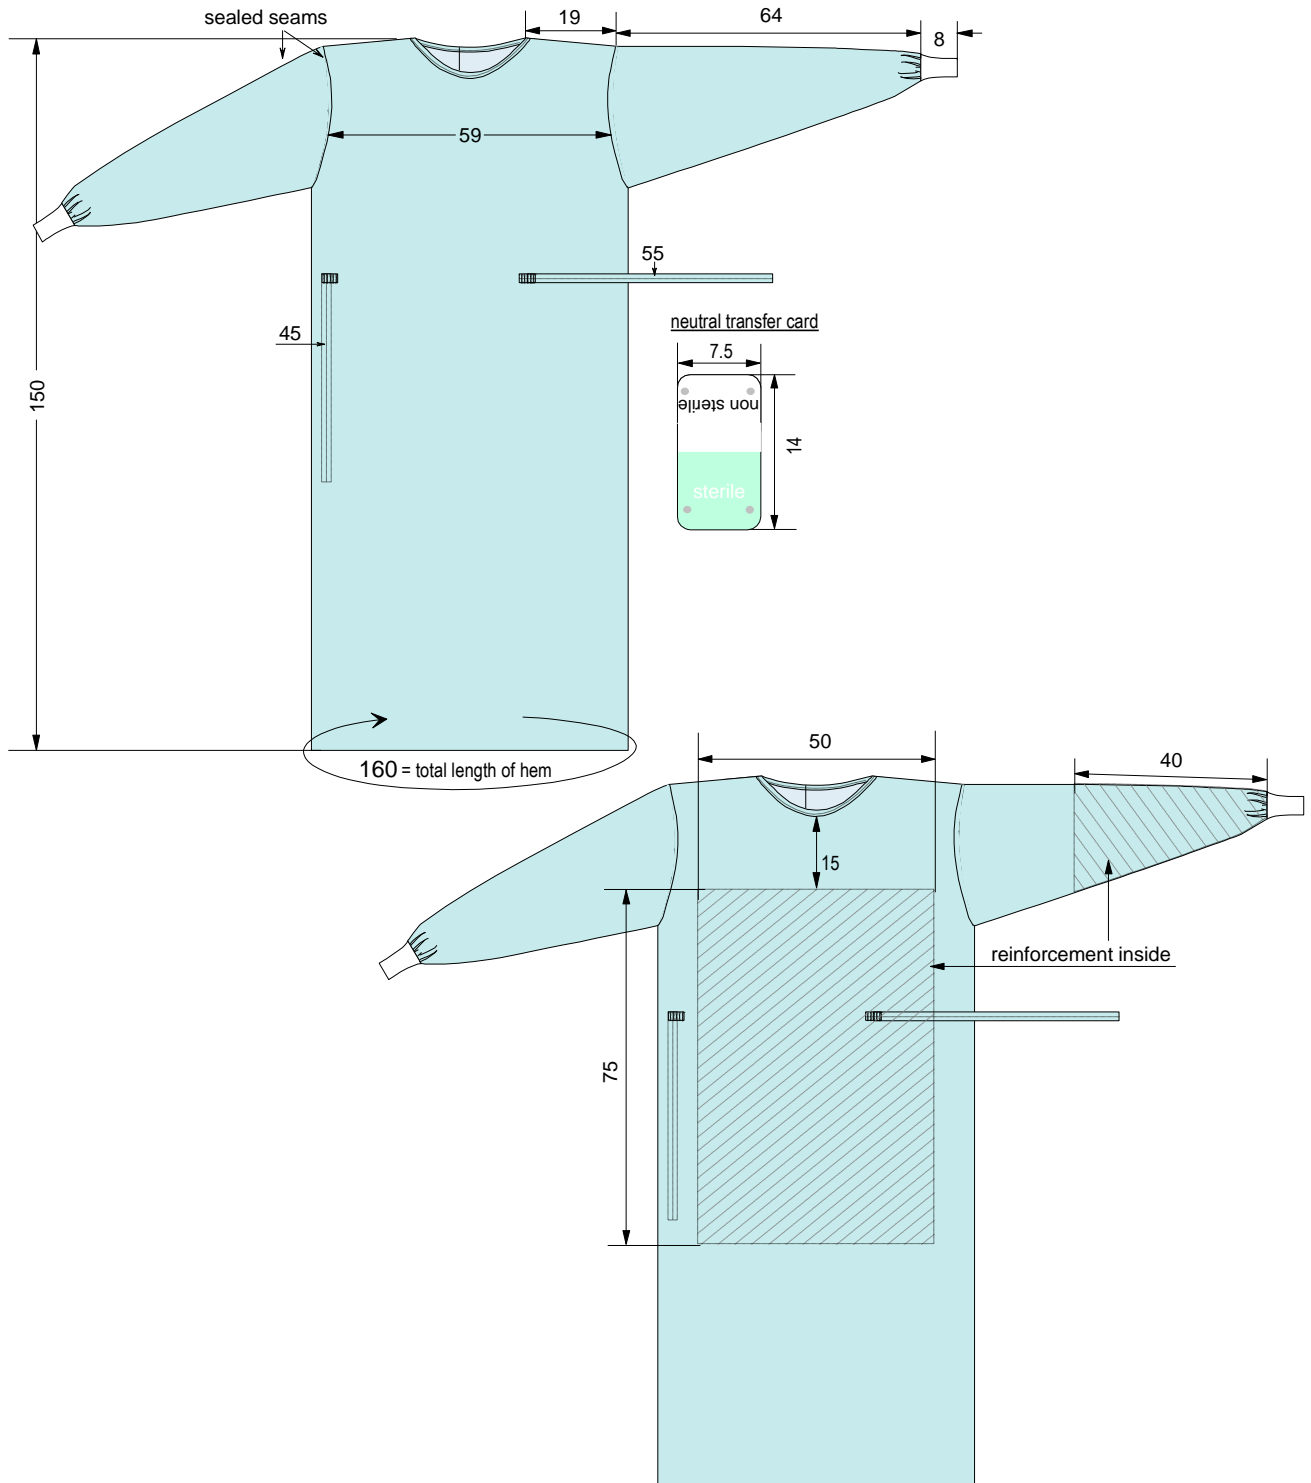


all dimensions in cm



Article OR Gown, Mediwell light
with Reinforcement, Standard Performance

Specification No. **46 44 37C**

7.1 Folding

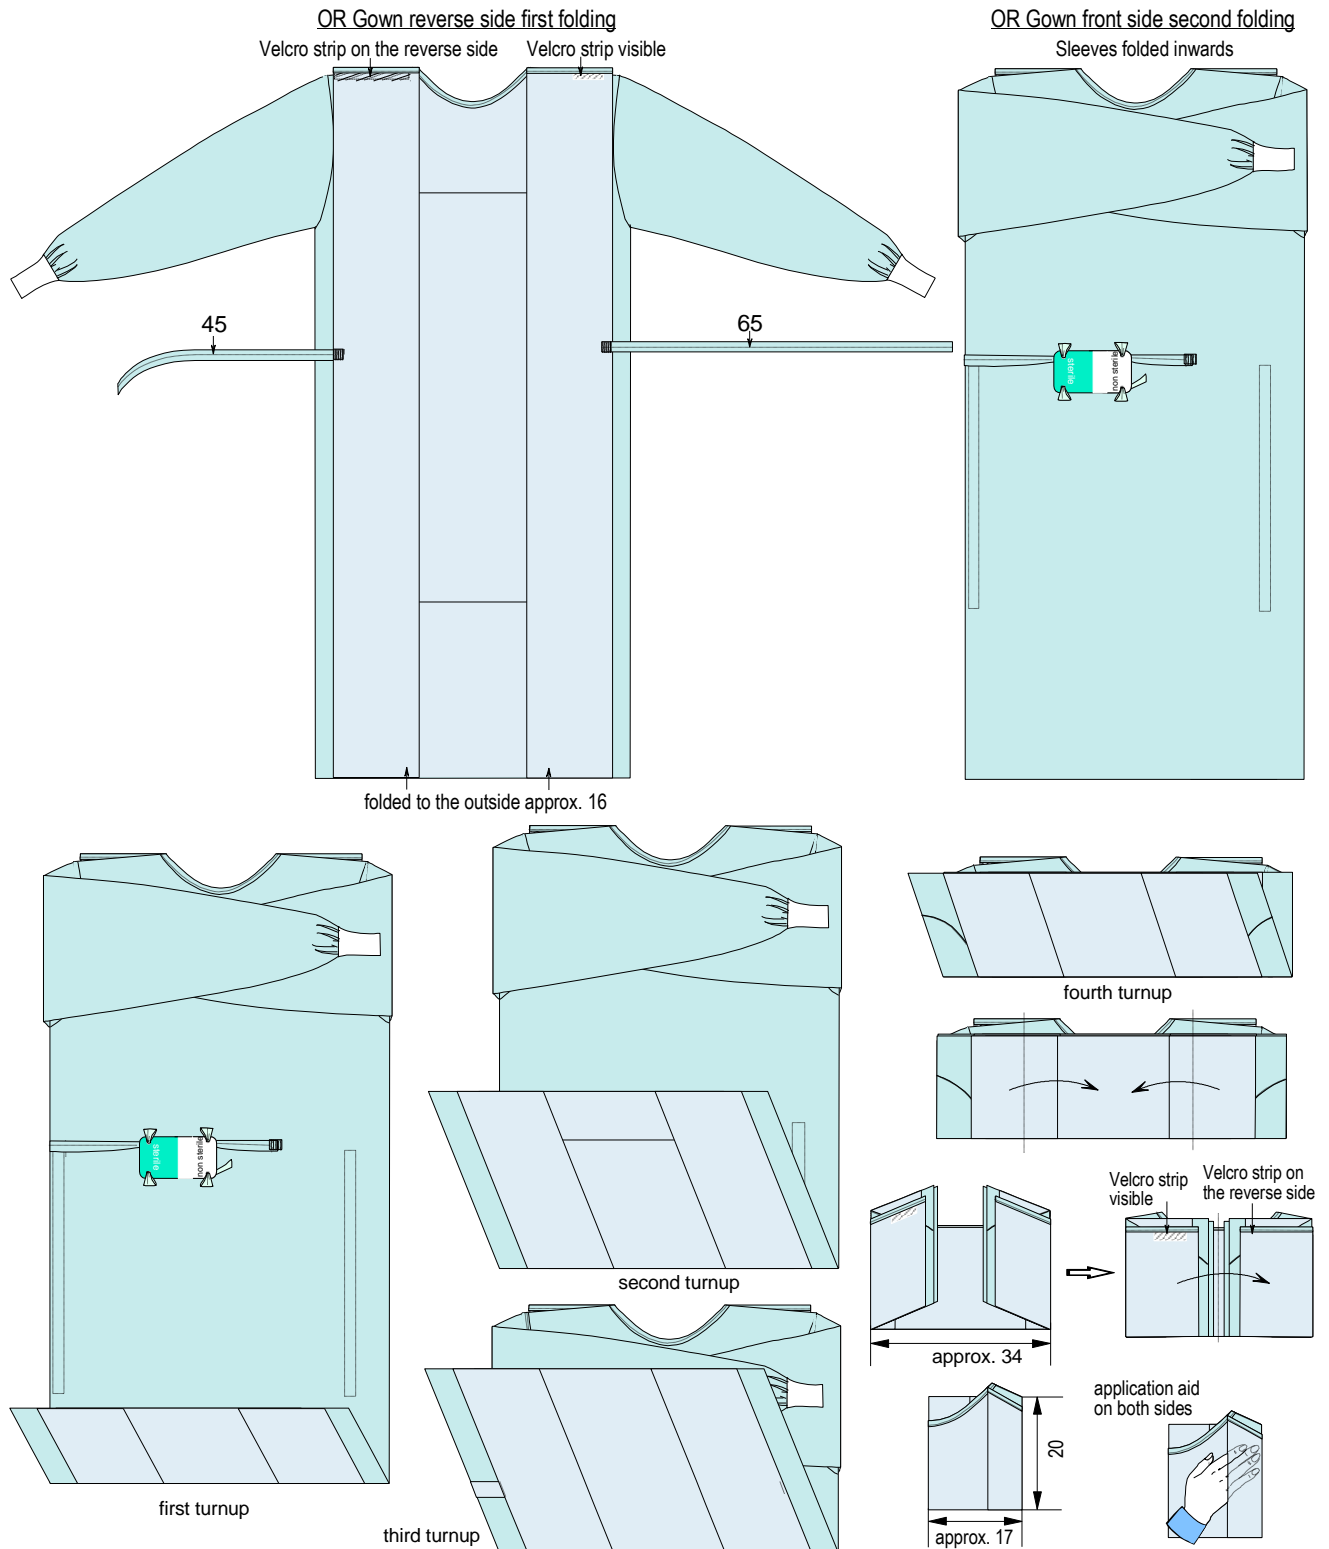


all dimensions in cm



Article OR Gown, Mediwell light
with Reinforcement, Standard Performance

Specification No. **46 44 37C**

7.2 Overwrap

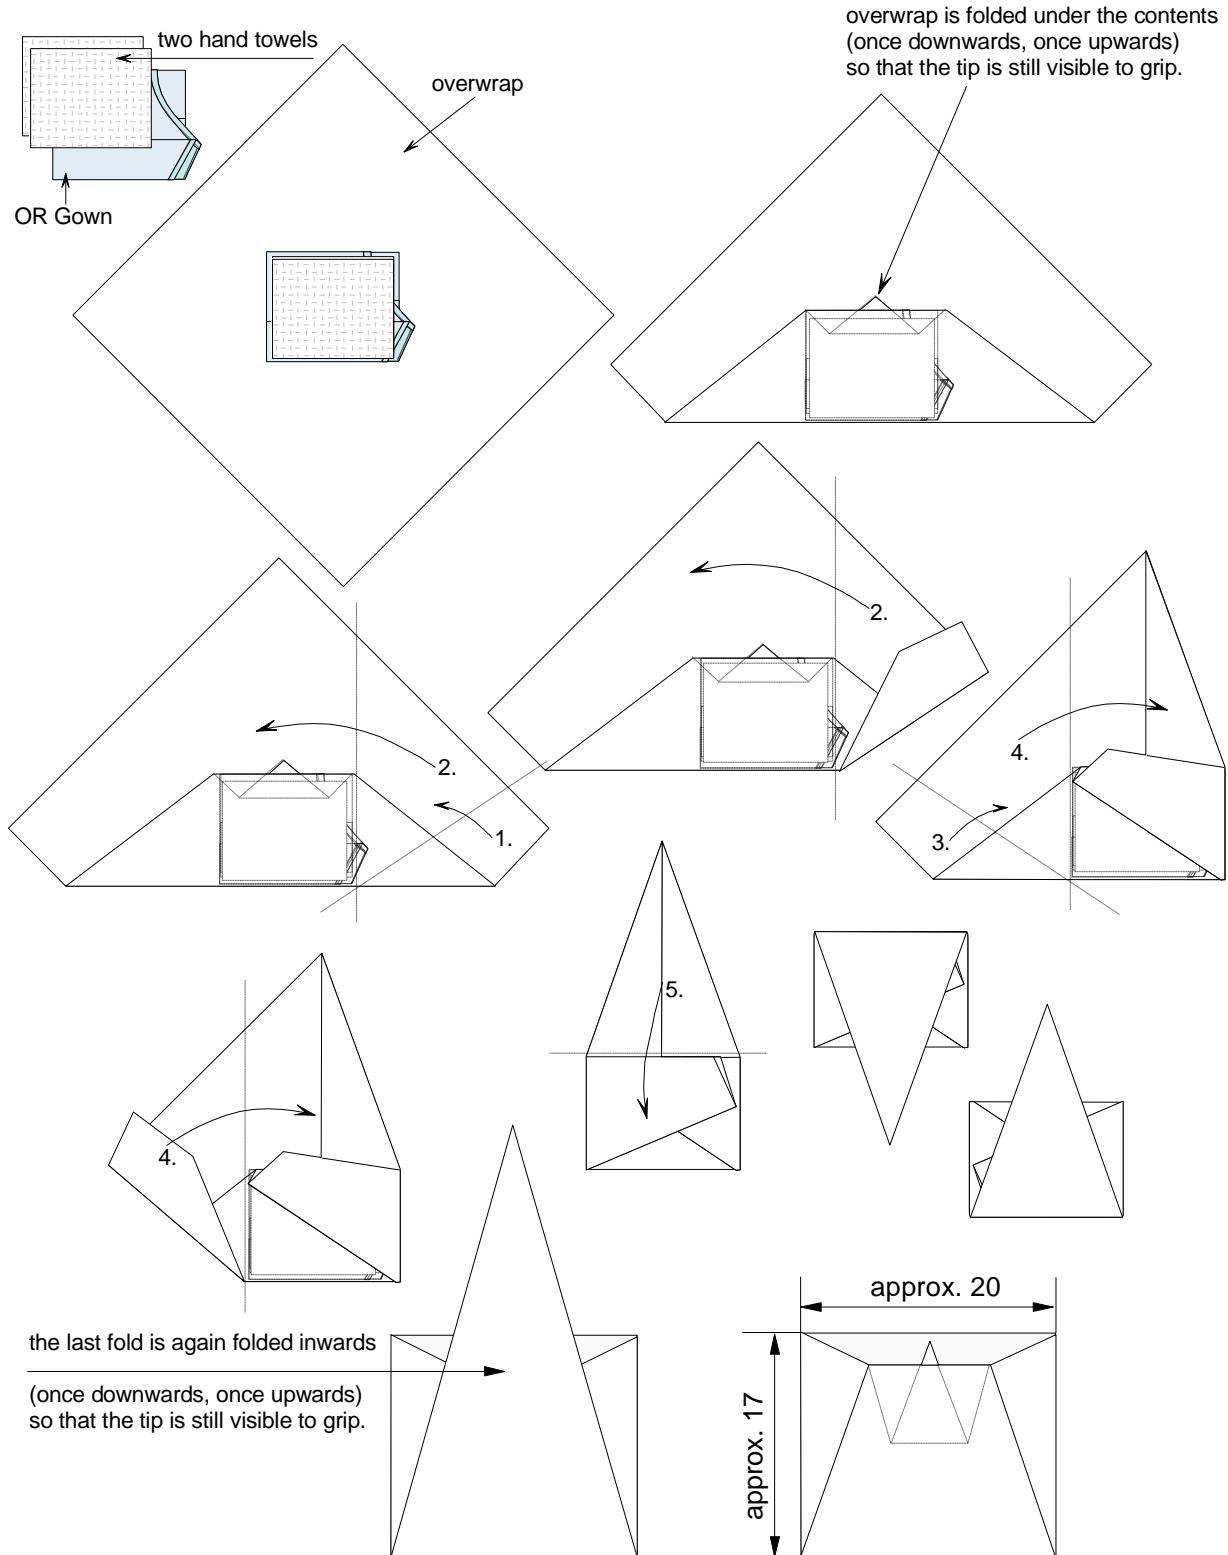

all dimensions in cm



Article	OR Gown, Mediwell light with Reinforcement, Standard Performance
Specification No.	46 44 37C
8. Packaging/ <i>sterile goods</i>	
8.1 Primary packaging	
• Paper	60 g/m ² ± 10 %
• Film	100 µm ± 10 %, transparent
8.2 Film bag	
• Size	500 / 300 x 700 mm ± 10 mm
• Film	PE film, 30µm, transparent
• Contents	14 pcs.
8.3 Transport packaging	
• Size	492 x 292 x 400 mm ± 10 mm
• Contents	28 (2 x 14) pcs.
8.4 Sterilisation	<i>EtO gas sterilisation (in accordance with ISO 11135)</i>
8.5 Usability and storage	5 years, no direct exposure to sunshine, store at a dry place.
9. Packaging / <i>non-sterile goods</i>	
9.1 Film bag 2x	
• Size	1.200 x 800 mm ± 10 mm
• Film	PE film 35 µm ± 10 %, transparent
9.2 Transport carton	
• Size	780 x 385 x 295 mm ± 10 mm
• Contents	50 pcs.
9.3 Sterilisation	suitable for sterilisation by EtO gas
9.4 Usability and storage	6 years, no direct exposure to sunshine, store at a dry place.
10. Disposal	The raw material can be disposed of in an environmentally friendly manner. No toxic gases are released during incineration. The ground water is not contaminated by toxic substances when dumped.

This product specification is the property of SENGEWALD Klinikprodukte GmbH and is to be treated with the strictest confidence. Communication to third parties and duplication, in whole or in part, are not permitted.